

Distal Rinse Procedure


1 50mL PBS with 0.02% Tween 80 (PBST) (Cat. no. U334)




2 Aseptically transfer contents to sterile 120mL specimen cup (Cat. no. PC4064200S)



3 Dip brush in PBST. Sample elevator mechanism, recess, and channel. Brush under elevator mechanism and scrub the camera lens. Deposit brush in PBST.

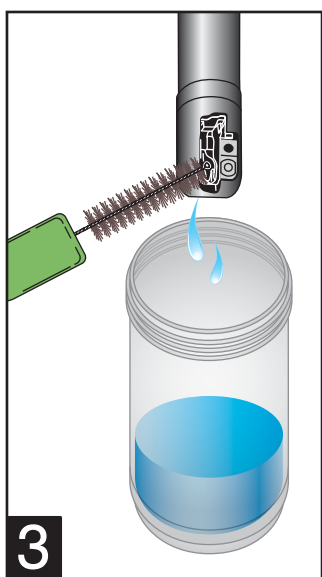

4 Tighten lid and seal with Parafilm. Hold sample at 4 °C until further processing.

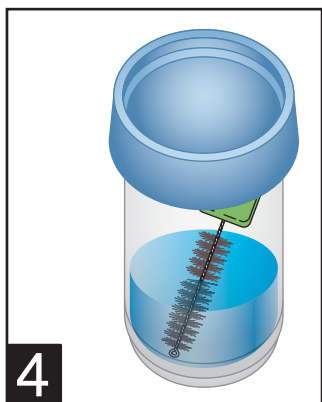

Channel Rinse Procedure


1 50mL sterile water (Cat. no. U336)




2 Aseptically transfer contents to sterile 120mL specimen cup (Cat. no. PC4064200S)



4 Flush instrument channel and collect contents in sterile 120mL specimen cup.

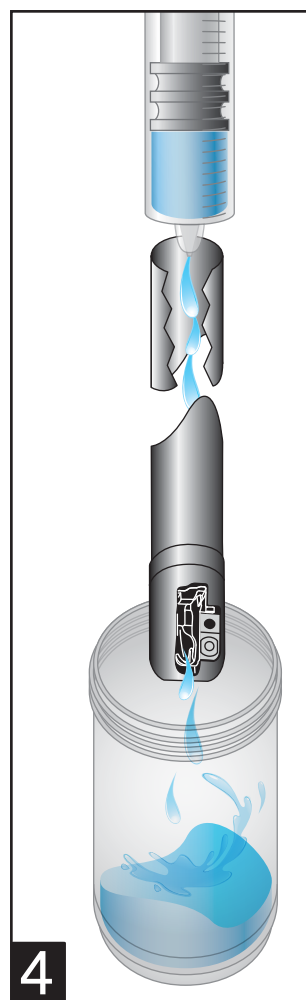

3 Withdraw the 50mL of water into a 60mL syringe.

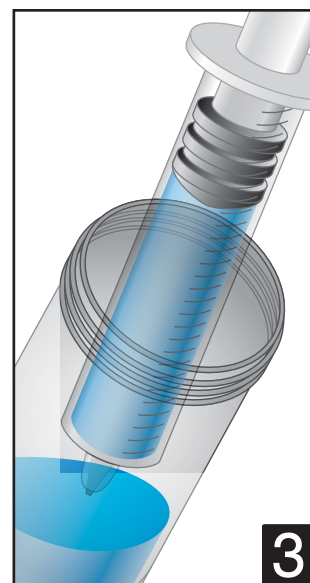

5 Tighten lid and seal with Parafilm. Hold sample at 4°C until further processing.

